


Controls

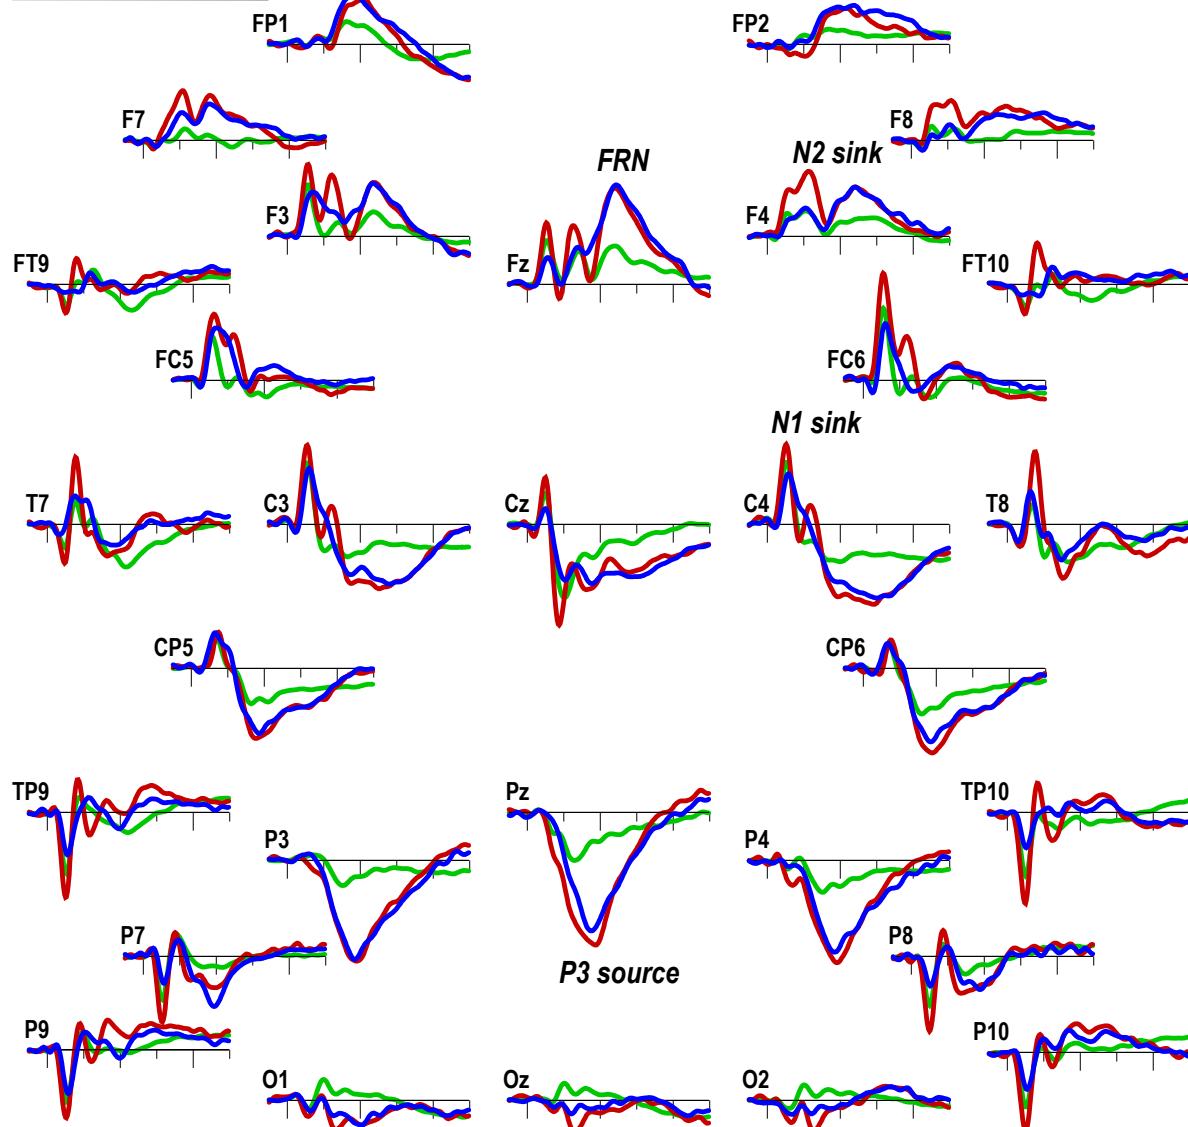



Current Source Density


0.1 μ V/cm²

— Tonal Target
— Phonetic Target
— Nontarget


↑
0 400 800
Latency [ms]

Patients

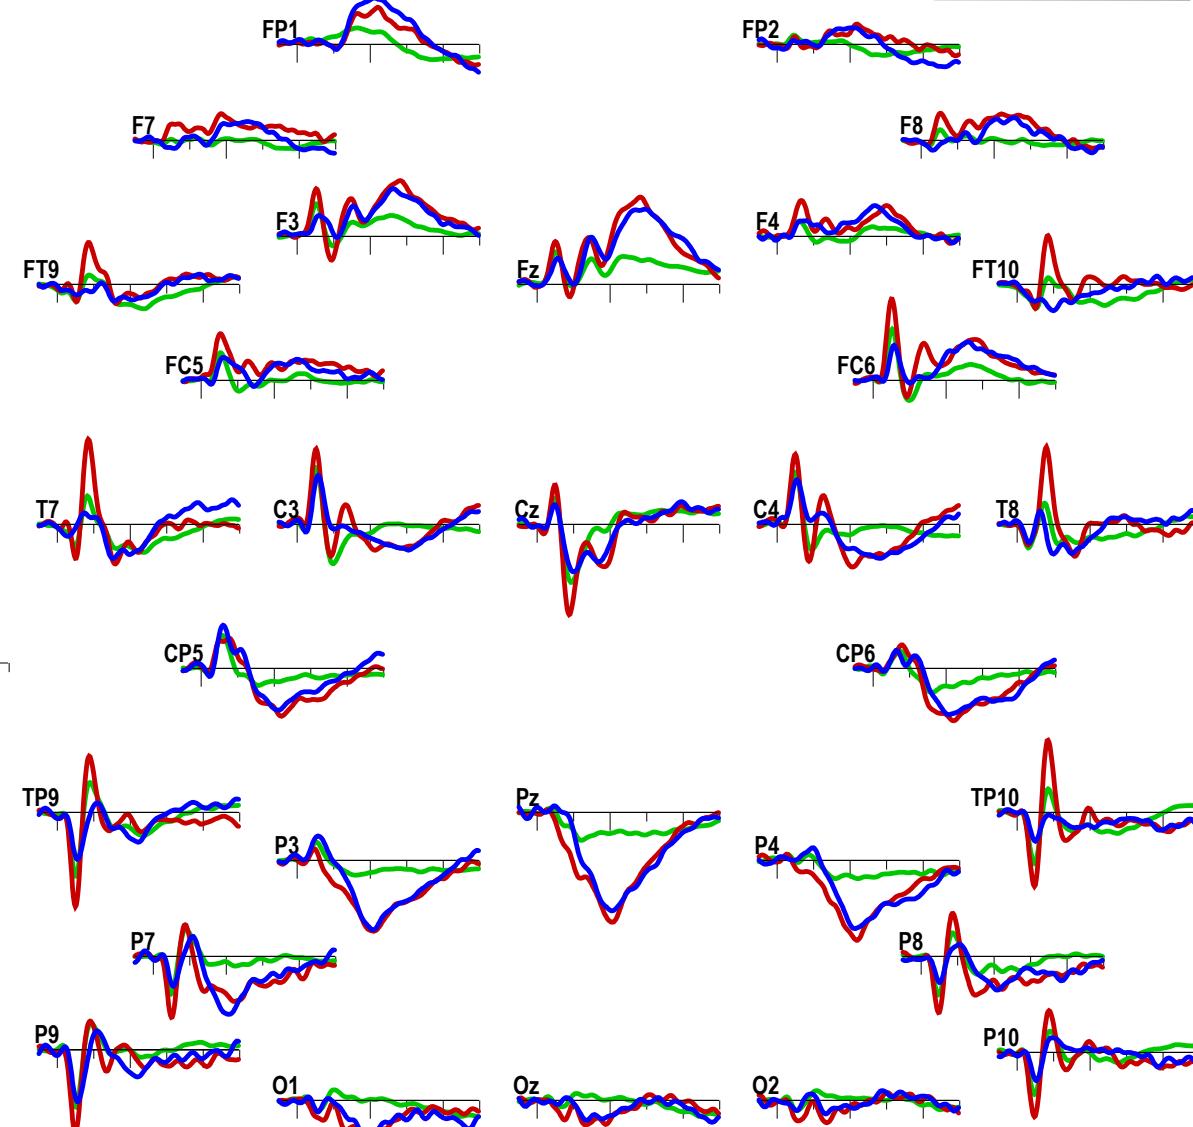



Controls

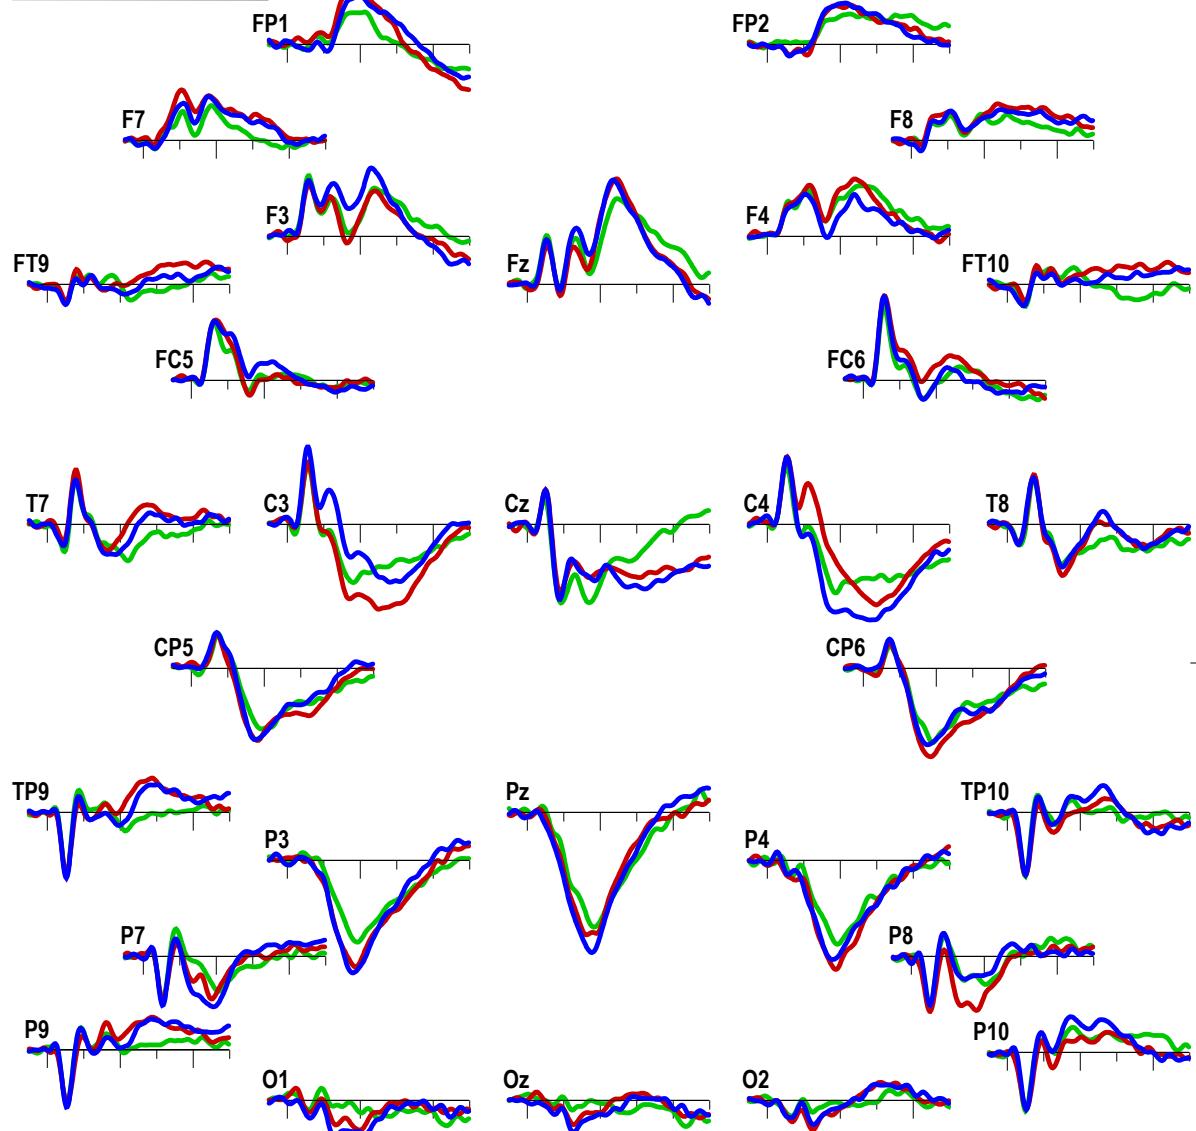

Current Source Density

$0.1 \mu\text{V}/\text{cm}^2$

- Left Press
- Right Press
- Silent Count

↑
0 400 800
Latency [ms]

Patients

